



Together with new optics, ECLIPSE is evolving to the next stage.

Modularized to meet industrial microscope applications in diverse fields of industry, including semiconductor devices, packaging, FPDs, electronic components, materials, and precision molds.

The ECLIPSE LV Series continues to evolve while offering various stand and illumination units selectable according to the observation method and purpose.

Four types – motorized and manual types plus dedicated reflected illumination and combined reflected/ transmitted illumination types – are available to meet any application.

Illuminators

Expanded lineup

Added a compact LED illuminator to the existing lineup.

With the use of LED, Nikon illuminators are power saving and achieve long life.



Evolved optical performance

Nikon's CFI₆₀ optical system, highly evaluated for its unique concept of high NA combined with long working distance has further evolved to achieve the apex in long working distance, chromatic aberration correction, and light weight.

Easy Operation

Combination with digital camera

Detection of microscope information, including objective lens information, and motorized unit microscope operation are now possible using imaging software, for more efficient observation and image capture.

Observation Methods

Diverse observation / optical contrast methods

Combinations of a full range of accessories expand the observation methods available when using transmitted illumination, allowing adaptability to a greater diversity of samples.

All models enable brightfield, darkfield, differential interference, fluorescence, polarizing, and two-beam interferometry observation, while the LV100ND and LV100NDA also allow transmission-type differential interference, darkfield, polarizing, and phase contrast observation.



LV-N Series

Model features









LV100ND

LV100NDA

Dedicated reflected illumination models

Microscope type

Compatible observation methods

Compatible stages

Manual type

Motorized type (Nosepiece)

		Brightfield	Darkfield	DIC	Fluorescence	Polarizing	Two-beam Interferometry
LV150/	Episcopic	0	0	0	0	0	0
LV150NA	Episcopic (LED)	0	0	0	_	Δ	_
LV150NL	Episcopic	0	_	0	_	0	0

- * Use an objective lens appropriate to the observation method.

 △: only simple polarizing observation
 - LV-S32 3x2 stage (Stroke: 75 x 50 mm with glass plate)
 *Can be fitted with LV-S32SPL ESD plate
 - LV-S6 6x6 stage (Stroke: 150 x 150 mm)
 - *Can be fitted with LV-S6WH wafer holder / LV-S6PL ESD plate
 - LV-SRP P revolving stage
 - P-GS2 G stage 2 (Used with stage adapter LV-SAD)

DS-Ri2 or DS-Fi3 + NIS-Elements (Microscope camera + imaging software)

Integration with Digital Sight cameras for microscopes

 Objective lens information detection (when used with combination of Intelligent Nosepiece LV-NU5I and LV-INAD) Objective lens information detection and control Elements

Combined reflected/transmitted illumination models

Manual type

Motorized type

(Nosepiece / light intensity / aperture stop / observation method selector)

		Brightfield	Darkfield	DIC	Fluorescence	Polarizing	Two-beam Interferometry	Phase- contrast
	Episcopic	0	0	0	0	0	0	_
LV100ND/ LV100DA-U	Episcopic (LED)	0	0	0	_	Δ	_	_
	Diascopic	0	0	0	_	0	_	0

- * Use an objective lens appropriate to the observation method.

 △: only simple polarizing observation
 - LV-S32 3x2 stage (Stroke: 75 x 50 mm with glass plate)
 *Can be fitted with LV-S32SGH slide glass holder
 - LV-S64 6x4 stage (Stroke: 150 x 100 mm with glass plate)
 - LV-SRP P revolving stage
 - P-GS2 G stage 2 (Used with stage adapter LV-SAD)
 - NIU-CSRR2 Ni-U right handle rotatable ceramic stage (Stroke: 78 x 54 mm)
 - C-SR2S right handle stage (Stroke: 78 x 54 mm: Used with stage adapter LV-SAD)

DS-Ri2 or DS-Fi3 + NIS-Elements (Microscope camera + imaging software)

 Objective lens information detection (when used with combination of Intelligent Nosepiece LV-NU5I and LV-INAD) Information detection and control of objective lens, light intensity, aperture stop, and observation method (brightfield / darkfield / fluorescence)

Elements

Evolved optical performance

Nikon's CFI60 optical systems are highly evaluated for their unique concept of high NA combined with a long working distance. These lenses have been developed further and evolved achieving the apex in long working distance specifications, correct chromatic aberration, and an optimized lens weight.

T Plan & TU Plan Fluor & TU Plan Apo Lenses

Standard Plan objective lenses

Standard objective lenses

TU Plan Fluor Series

EPI/BD 5x/10x/20x/50x/100x

Enable brightfield, darkfield, simple polarizing, sensitive polarizing, differential interference, and epi-fluorescence observations with just one lens. Achieves superior chromatic aberration performance with long working distance for all magnifications to adapt to any application.



*Brightfield observation (EPI) objective lens

Model	Magnification	NA	Working Distance (mm)
TU Plan Fluor EPI	5×	0.15	23.5
(brightfield type)	10×	0.30	17.5
	20×	0.45	4.5
	50×	0.80	1.0
	100×	0.90	1.0
TU Plan Fluor BD	* 5×	0.15	18.0
(brightfield/darkfield type)	* 10×	0.30	15.0
	* 20×	0.45	4.5
	50×	0.80	1.0
	100×	0.90	1.0

^{*} Uses fly-eye lens.

Low-magnification objective lenses

T Plan EPI

EPI 1x/2.5x

Both clear observation using a conventional analyzer/polarizer and operability-oriented observation without the need of an analyzer/ polarizer are possible.



Model	Magnification	NA	Working Distance (mm)
T Plan EPI	1×	0.03	3.8
(brightfield type)	2.5×	0.075	6.5

Apochromatic objective lenses

TU Plan Apo Series EPI/BD 50x/100x/150x

By using phase Fresnel lenses, these objective lenses achieve significantly longer operating distances while maintaining the superior chromatic aberration performance of apochromatic




*Brightfield observation (EPI) objective lens

Model	Magnification	NA	Working Distance (mm)
TU Plan Apo EPI	50×	0.8	2.0
(brightfield type)	100×	0.9	2.0
	150×	0.9	1.5
TU Plan Apo BD	50×	0.8	2.0
(brightfield/darkfield type)	100×	0.9	2.0
	150×	0.9	1.5

Dark Field Illumination

Fly-eye lens


Through the use of fly-eye lenses, the CFI60-2 optical system offers bright darkfield illumination throughout the field of view with little unevenness, even for lowmagnification lenses.



Fly-eye lenses adjust the diffusion angle of light so light strikes the focal

Darkfield illumination system ·····

As NA and WD improve, objective lenses increase in outside diameter. However, as the width of incident light is fixed, light intensity decreases with conventional illumination systems The illumination system uses annular lenses or annular prisms to increase captured light and achieve bright darkfield illumination with no deterioration



more light to increase brightness

TU Plan ELWD & T Plan SLWD Lenses

Long working distance objective lenses

TU Plan ELWD Series

EPI/BD 20x/50x/100x

With the phase Fresnel lenses, these objective lenses enable long working distances while offering higher level chromatic aberration correction than conventional objective lenses. This improves operability for samples with

different heights.	proo mar	
Model	Magnification	
TU Plan EPI ELWD	20×	
(brightfield type)	50×	


Model	Magnification	NA	Working Distance (mm)
TU Plan EPI ELWD	20×	0.4	19.0
(brightfield type)	50×	0.6	11.0
	100×	0.8	4.5
TU Plan BD ELWD	20×	0.4	19.0
(brightfield/darkfield type)	50×	0.6	11.0
	100×	0.8	4.5

Super-long working distance objective lenses

Long working distance / Super-long working distance objective lenses

T Plan EPI SLWD

10x/20x/50x/100x












Model	Magnification	NA	Working Distance (mm)
T Plan EPI SLWD	10×	0.2	37.0
(brightfield type)	20×	0.3	30.0
	50×	0.4	22.0
	100×	0.6	10.0

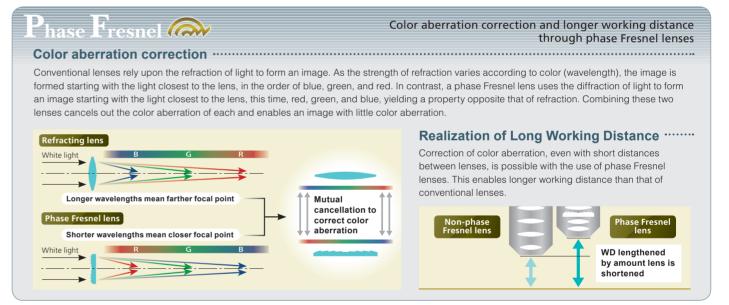

*Brightfield observation

(EPI) objective lens

Other lenses

Objective lenses with glass thickness correction features

CFI L Plan EPI CR 20x/50x/100x

Equipped with corrective features that enable high contrast observation of cells or patterns, these observation lenses are unaffected by the glass substrate.



Model	Magnification	NA	Working Distance (mm)
CFI L Plan EPI CR	20× CR	0.45	10.90 - 10.00
(brightfield type)	50× CR	0.70	3.90 - 3.00
	100× CRA	0.85	1.20 - 0.85
	100x CBB	0.85	1 30 - 0 95

Objective lenses for brightfield/darkfield observation

CFI LE Plan EPI/BD EPI 5x/10x/20x/50x/100x BD 5x/10x/20x/50x/







Model	Magnification	NA	Working Distance (mm)
LE Plan EPI	5×	0.1	31.0
(brightfield type)	10×	0.25	13.0
	20×	0.4	3.6
	50×	0.75	0.5
	100×	0.9	0.31
LE Plan BD	5×	0.1	18.0
(brightfield/darkfield type)	10×	0.25	13.0
	20×	0.4	3.6
	50~	0.75	0.5

7

Easy Operation

Combination with digital camera

LV150N/LV100ND/LV150NA

Objective lens information detection and control


Information about the objective lens being used can be detected when combining the Intelligent Nosepiece LV-NU5I and the Nosepiece Adaptor LV-INAD. The information is automatically converted to appropriate calibration data when changing the magnification.

In addition, the LV150NA allows switching of objective lenses via the imaging software.






LV-INAD Nosepiece Adaptor

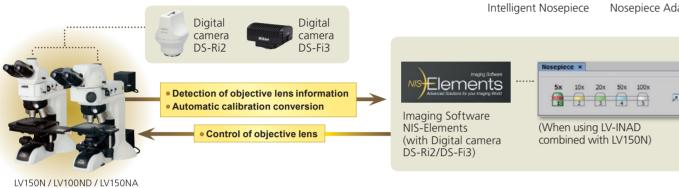

LV100NDA

Microscope information detection and control

The LV100NDA allows detection of information and control of objective lenses, light intensity, aperture stop, and observation method (brightfield / darkfield / fluorescence) via the imaging software, enabling optimization of the conditions vital for image acquisition.

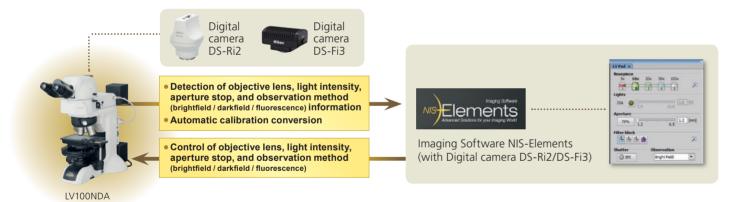


⊚: Information detection and control possible ○: Information detection only	LV150N/LV100ND (When using LV-NU5I and LV-INAD)	LV150NA	LV100NDA (When using LV-UEPI2A Illuminator
O. Illiornation detection only	DS-Ri2/DS-Fi3 (+NIS-Elements)	DS-Ri2/DS-Fi3 (+NIS-Elements)	DS-Ri2/DS-Fi3 (+NIS-Elements)
Objective lens	0	<u></u>	<u></u>
Reflected illumination *When using (ON/OFF, light intensity adjustment) LV-LH50PC		_	0
Transmitted illumination (ON/OFF, light intensity adjustment)	_	<u>—</u>	<u></u>
Aperture stop			0
Observation method selector (brightfield / darkfield / fluorescence)	<u>—</u>	<u>—</u>	<u></u>

Note: With NIS-Elements L and F, functions above are not available. Use NIS-Elements D/Br/Ar.

Camera System

Digital camera system for microscopes "Digital Sight System"




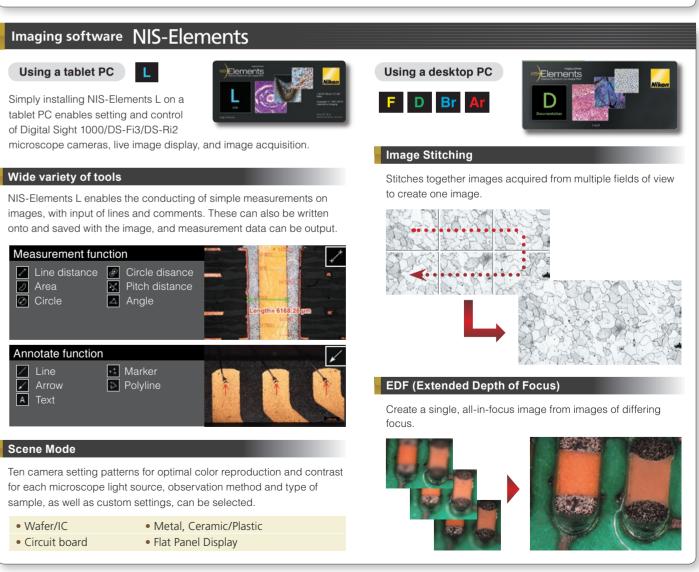

^{*} See the "Digital Camera Digital Sight Series for Microscopes" brochure for details on Digital Sight features.


Observation Methods

Compatible with a wide range of observation / optical contrast methods: In reflected light mode -brightfield, darkfield, polarizing, differential interference, epi-fluorescence, and two-beam interferometry, and in Transmitted light mode- brightfield, darkfield, polarizing, differential interference, and phase contrast.




Semiconductors (IC wafers)

From its objective lenses to its illumination systems, the LV-N Series offers thorough measures against flare and provides bright, high-contrast images.




Substrate (solder)

The LV-N Series demonstrates superiority in the observation of samples with fluorescent properties, such as organic ELs or mounted substrates.



LCD (color filter)

The LV-N Series is effective in the observation of samples with transparency, such as optical components, FPDs, and slide glass samples. When used in conjunction with the C-SP Simple Polarizer and analyzers, transmitted simple polarized observation is possible.



Semiconductors (IC wafers)

The use of Nikon's unique concepts in the objective lens darkfield illumination system enables bright darkfield observation and provides high-sensitivity detection of level differences and defects in samples.



Minerals


Briahtfield)

The LV-N Series is effective in the observation of samples with birefringent properties, such as liquid crystals or plastics/glass containing distortion.



Substrate

Standard-type and high-contrast-type DIC sliders are available to match samples. The LV-N Series is effective for applications such as observation of minute level differences in devices and precision molds.



Mica

Michelson (TI) and Mirau (DI) reflection-type two-beam interferometry is possible with the LV-N Series. When used with micrometer eyepieces, minute level differences can be detected and measured without contact with the sample.



Emulsion

Colorless, transparent samples can be made visible through bright/dark contrast and the use of diffraction and interference, two properties of light.



Nanoparticle (silver)

Colorless, transparent samples can be observed in three dimensions by using polarization to create interference between two beams of light.

Specifications

	LV150N	LV150NA	LV150NL
Base unit	Maximum sample height: 38 mm (when used wand LV-S32 3x2 stage / LV-S64 6x4 stage) * 73 mm when used with one column riser 12V50W internal power source for dimmer, coa Left: coarse and fine adjustment / Right: fine ac Coarse adjustment: 14 mm/turn (with torque ac mechanism) Fine adjustment: 0.1 mm/turn (1) Stage mounting hole intervals: 70 x 94 (fixed b)	arse and fine adjustment knobs djustment, 40 mm stroke djustment, refocusing µm/graduation)	Maximum sample height: 38 mm (when used with LV-S32 3x2 stage) * 73 mm when used with one column riser Internal LED illumination power source, coarse and fine adjustment knobs Left: coarse and fine adjustment / Right: fine adjustment, 40mm stroke Coarse adjustment: 14 mm/turn (with torque adjustment, refocusing mechanism) Fine adjustment: 0.1 mm/turn (1 µm/graduation) Stage mounting hole intervals: 70 x 94 (fixed by 4-M4 screw)
Nosepieces	C-N6 ESD Sextuple Nosepiece ESD LV-NU5 Universal Quintuple Nosepiece ESD LV-NBD5 BD Quintuple Nosepiece ESD LV-NU5I Intelligent Universal Quintuple Nosepiece ESD	LV-NU5A Motorized Universal Quintuple Nosepiece ESD LV-NU5AC Motorized Universal Quintuple Nosepiece ESD	C-N6 ESD Sextuple Nosepiece ESD LV-NU5 Universal Quintuple Nosepiece ESD
Episcopic Illuminator	LV-UEPI-N LV-LH50PC 12V50W Precentered Lamphouse, LV-LL LED Lamphouse Bright/darkfield switch and linked aperture stop (centerable), field diaphragm (centerable) Accepts Ø 25 mm filter (NCB11, ND16, ND4), polarizer/analyzer, λ plate, excitation light balancer; equipped with noise terminator		1.1W white LED Accepts polarizer/analyzer
	LV-UEPI2 LV-LH50PC 12V50W Precentered Lamphouse HG precentered fiber illuminator: C-HGFIE (wit Bright/darkfield switch and linked aperture sto; (centerable), automated optical element switch brightfield, darkfield, and epi-fluorescence switch Accepts of 25 mm filter (NCB11, ND16, ND4), p excitation light balancer; equipped with noise t	h light adjustment) *option p (centerable), field diaphragm ning feature matched to tch olarizer/analyzer, λ plate,	
Eyepiece tubes	LV-TI3 trinocular eyepiece tube ESD (Erected image, FOV: 22/25) LV-TT2 TT2 tilting trinocular eyepiece tube (Erected image, FOV: 22/25) C-TB binocular tube (Inverted image, FOV: 22) P-TB Binocular Tube (Inverted image, FOV: 22) P-TT2 Trinocular Tube (Inverted image, FOV: 22)		LV-TI3 trinocular eyepiece tube ESD (Erected image, FOV: 22/25) C-TB binocular tube (Inverted image, FOV: 22) P-TB Binocular Tube (Inverted image, FOV: 22) P-TT2 Trinocular Tube (Inverted image, FOV: 22)
Stages	LV-S32 3x2 stage (Stroke: 75 x 50 mm with glass plate) ESD compatible LV-S64 6x4 stage (Stroke: 150 x 100 mm with glass plate) ESD compatible LV-S6 6x6 stage (Stroke: 150 x 150 mm) ESD compatible		LV-S32 3x2 stage (Stroke: 75 x 50 mm with glass plate) ESD compatible LV-S6 6x6 stage (Stroke: 150 x 150 mm) ESD compatible
Eyepieces	CFI eyepiece series		
Objective lenses	Industrial Microscope CFI60-2/CFI60 optical sys	stem Objective lens series: Combi	nations in accordance with the observation method
ESD performance	1,000 to 10V, within 0.2 sec. (excluding certain	accessories)	
Power consumption	1.2 A / 75 W		0.1A / 3W
Weight	Approx. 8.6 kg	Approx. 8.7 kg	Approx. 8.6 kg

	LV100ND	LV100NDA				
Base unit	Maximum sample height: 38 mm (when used with LV-NU5 U5 nosepiece and LV-S32 3x2 stage / LV-S64 6x4 stage) 12V50W internal power source for dimmer, coarse and fine adjustment knobs Left: coarse and fine adjustment / Right: fine adjustment, 40 mm stroke Coarse adjustment: 14 mm/turn (with torque adjustment, refocusing mechanism) Fine adjustment: 0.1 mm/turn (1 µm/graduation)	Maximum sample height: 33 mm (when used with LVNU5AI U5AI nosepiece and LV-S32 3x2 stage / LV-S64 6x4 stage) 12V50W internal power source for dimmer, coarse and fine adjustment knobs Left: coarse and fine adjustment / Right: fine adjustment, 40 mm stroke Coarse adjustment: 14 mm/turn (with torque adjustment, refocusing mechanism Fine adjustment: 0.1 mm/turn (1 μm/graduation)				
Nosepieces	C-N6 ESD Sextuple Nosepiece ESD, LV-NU5 Universal Quintuple Nosepiece ESD LV-NBD5 BD Quintuple Nosepiece ESD, LV-NU5I Intelligent Universal Quintuple Nosepiece ESD D-ND6 Sextuple DIC Nosepiece	LV-NU5AI Motorized Universal Quintuple Nosepiece (High-durability motorized 5-hole universal nosepiece)				
Episcopic Illuminators	LV-UEPI-N LV-LH50PC 12V50W Precentered Lamphouse, LV-LL LED Lamphouse Bright/darkfield switch and linked aperture stop (centerable), field diaphragm (centerable), accepts σ 25 mm filter (NCB11, ND16, ND4), polarizer/analyzer; equipped with noise terminator LV-UEPI2 LV-LH50PC 12V50W Precentered Lamphouse, LV-LL LED Lamphouse HG precentered fiber illuminator: C-HGFIE (with light adjustment) *option Bright/darkfield switch and linked aperture stop (centerable), field diaphragm (centerable), automated optical element switching feature matched to brightfield, darkfield, and epi-fluorescence switch Accepts σ 25 mm filter (NCB11, ND16, ND4), polarizer/analyzer, λ plate, excitation light balancer; equipped with noise terminator	LV-UEPI2A LV-LH50PC 12V50W Precentered Lamphouse, LV-LL LED Lamphouse HG precentered fiber illuminator: C-HGFIE (with light adjustment: PC controlled) *option Motorized operation and control of illumination selector turret Motorized aperture stop linked to bright/darkfield selector (automatic optimization matched to objective lens), field diaphragm (centerable) Accepts Ø 25 mm filter (NCB11, ND16, ND4), polarizer/analyzer, λ plate, excitation light balancer; equipped with noise terminator				
Diascopic Illuminator	LV-LH50PC 12V50W Precentered Lamphouse (Fly Eye optical system) Internal aperture, field diaphragm, filter (ND8, NCB11); transmitted/reflected selector switch; 12V100W also available (option)					
Eyepiece tubes	LV-TI3 trinocular eyepiece tube ESD (Erected image, FOV: 22/25), LV-TT2 TT2 tilting trinocular eyepiece tube (Erected image, FOV: 22/25), P-TB Binocular Tube (Inverted image, FOV: 22), P-TT2 Trinocular Tube (Inverted image, FOV: 22)					
Stages	LV-S32 3x2 stage (Stroke: 75 x 50 mm with glass plate) / LV-S32SGH slide glass holder LV-S64 6x4 stage (Stroke: 150 x 100 mm with glass plate), LV-SRP P revolving stage / P-GS2 revolving stage: Used with stage adapter LV-SAD NIU-CSRR2 Ni-U right handle rotatable ceramic stage (Stroke: 78 x 54 mm), C-SR2S right handle stage (Stroke: 78 x 54 mm: Used with stage adapter LV-SAD)					
Condensers	LWD achromat condenser (brightfield), LV-CUD U condenser dry (phase contrast, diascopic DIC, darkfield), Achromat 2x-100x slide condenser (brightfield), DF dry condenser (darkfield), and others					
Eyepieces	CFI eyepiece series					
Objective lenses	Industrial Microscope CFI ₆₀ -2/CFI ₆₀ optical system Objective lens series: Combinations in accordance with the observation method					
ESD performance	1,000 to 10V, within 0.2 sec. (excluding certain accessories)					
Power consumption	1.2 A / 75 W	1.2 A / 90 W				
Weight	Approx. 9.5 kg	Approx. 10 kg				


Lens Specifications


	Туре	Model	Magnification	Product Code No.	NA	Working Distance (mm)
	Brightfield	T Plan EPI Plan (Semi-apochromat)	1×	MUE12010	0.03	3.8
			2.5×	MUE12030	0.075	6.5
		TU Plan Fluor EPI	5×	MUE12050	0.15	23.5
		Universal Plan Fluor (Semi-apochromat)	10×	MUE12100	0.3	17.5
			20×	MUE12200	0.45	4.5
			50×	MUE12500	0.8	1.0
			100×	MUE12900	0.9	1.0
		TU Plan Apo EPI Universal Plan Apo (Apochromat)	50×	MUC11500	0.8	2.0
			100×	MUC11900	0.9	2.0
			150×	MUC11150	0.9	1.5
	Polarizing	TU Plan Fluor EPI P Polarizing Universal Plan Fluor (Semi-apochromat)	5×	MUE13050	0.15	23.5
			10×	MUE13100	0.3	17.5
			20×	MUE13200	0.45	4.5
			50×	MUE13500	0.8	1.0
CFI 60-2			100×	MUE13900	0.9	1.0
	Brightfield Long Working Distance	TU Plan EPI ELWD Long Working Distance Universal Plan (Semi-apochromat)	20×	MUE21200	0.4	19.0
			50×	MUE21500	0.6	11.0
			100×	MUE21900	0.8	4.5
	Brightfield Super-long Working Distance	T Plan EPI SLWD Super-long Working Distance Plan (Semi-apochromat)	10×	MUE31100	0.2	37.0
			20×	MUE31200	0.3	30.0
			50×	MUE31500	0.4	22.0
			100×	MUE31900	0.6	10.0
	Brightfield/Darkfield	TU Plan Fluor BD Universal Plan Fluor (Semi-apochromat)	5×	MUE42050	0.15	18.0
			10×	MUE42100	0.3	15.0
			20×	MUE42200	0.45	4.5
			50×	MUE42500	0.8	1.0
			100×	MUE42900	0.9	1.0
		TU Plan Apo BD Universal Plan Apo (Apochromat)	50×	MUC41500	0.8	2.0
			100×	MUC41900	0.9	2.0
			150×	MUC41150	0.9	1.5
	Brightfield/Darkfield Long Working Distance	TU Plan BD ELWD Long Working Distance Universal Plan (Semi-apochromat)	20×	MUE61200	0.4	19.0
			50×	MUE61500	0.6	11.0
			100×	MUE61900	0.8	4.5


Phase Fresnel lens (diffraction optical element) type
 A circular polarizing plate and depolarizer are built into T Plan EPI 1x/2.5x. (Circular polarizing plate can be attached/detached.)


	Туре	Model	Magnification	Product Code No.	NA	Working Distance (mm)
CFI60	Brightfield With Correction Mechanism	L Plan EPI CR For Inspecting LCDs Plan	20×	MUE35200	0.45	10.9 - 10.0
			50×	MUE35500	0.7	3.9 - 3.0
			100×	MUE35900	0.85	1.2 - 0.85
			100×	MUE35910	0.85	1.3 - 0.95
	Brightfield	L Plan EPI Plan (Achromat)	40×	MUE00400	0.65	1.0
	Brightfield	LU Plan Apo EPI Universal Plan Apo (Apochromat)	100×	MUC00090	0.95	0.4
			150×	MUC10151	0.95	0.3
	Brightfield/Darkfield	LU Plan Apo BD Universal Plan Apo (Apochromat)	100×	MUC40900	0.9	0.51
			150×	MUC50151	0.9	0.42
	Brightfield	LE Plan EPI (Achromat)	5×	MUD00050	0.1	31.0
			10×	MUD00100	0.25	13.0
			20×	MUD00200	0.4	3.6
			50×	MUD00500	0.75	0.5
			100×	MUD00900	0.9	0.31
	Brightfield/Darkfield	LE Plan BD (Achromat)	5×	MUD10050	0.1	18.0
			10×	MUD10100	0.25	13.0
			20×	MUD10200	0.4	3.6
			50×	MUD10500	0.75	0.5

Dimensions

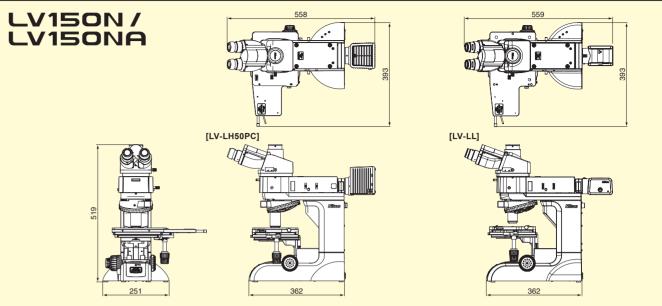

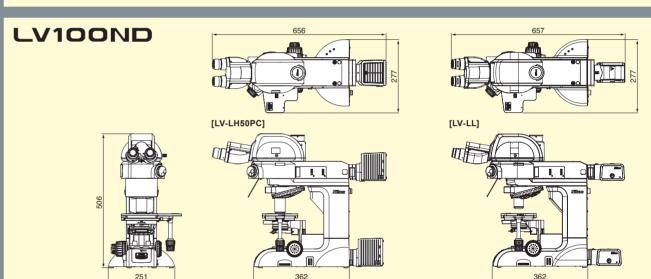

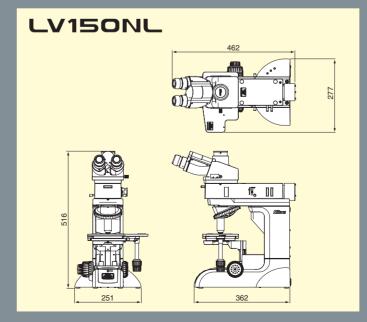


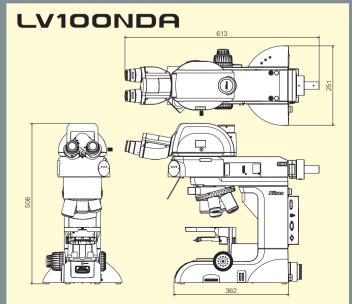

12

System Diagram


for LV150N/LV150ND/LV100NDA/LV100NDA

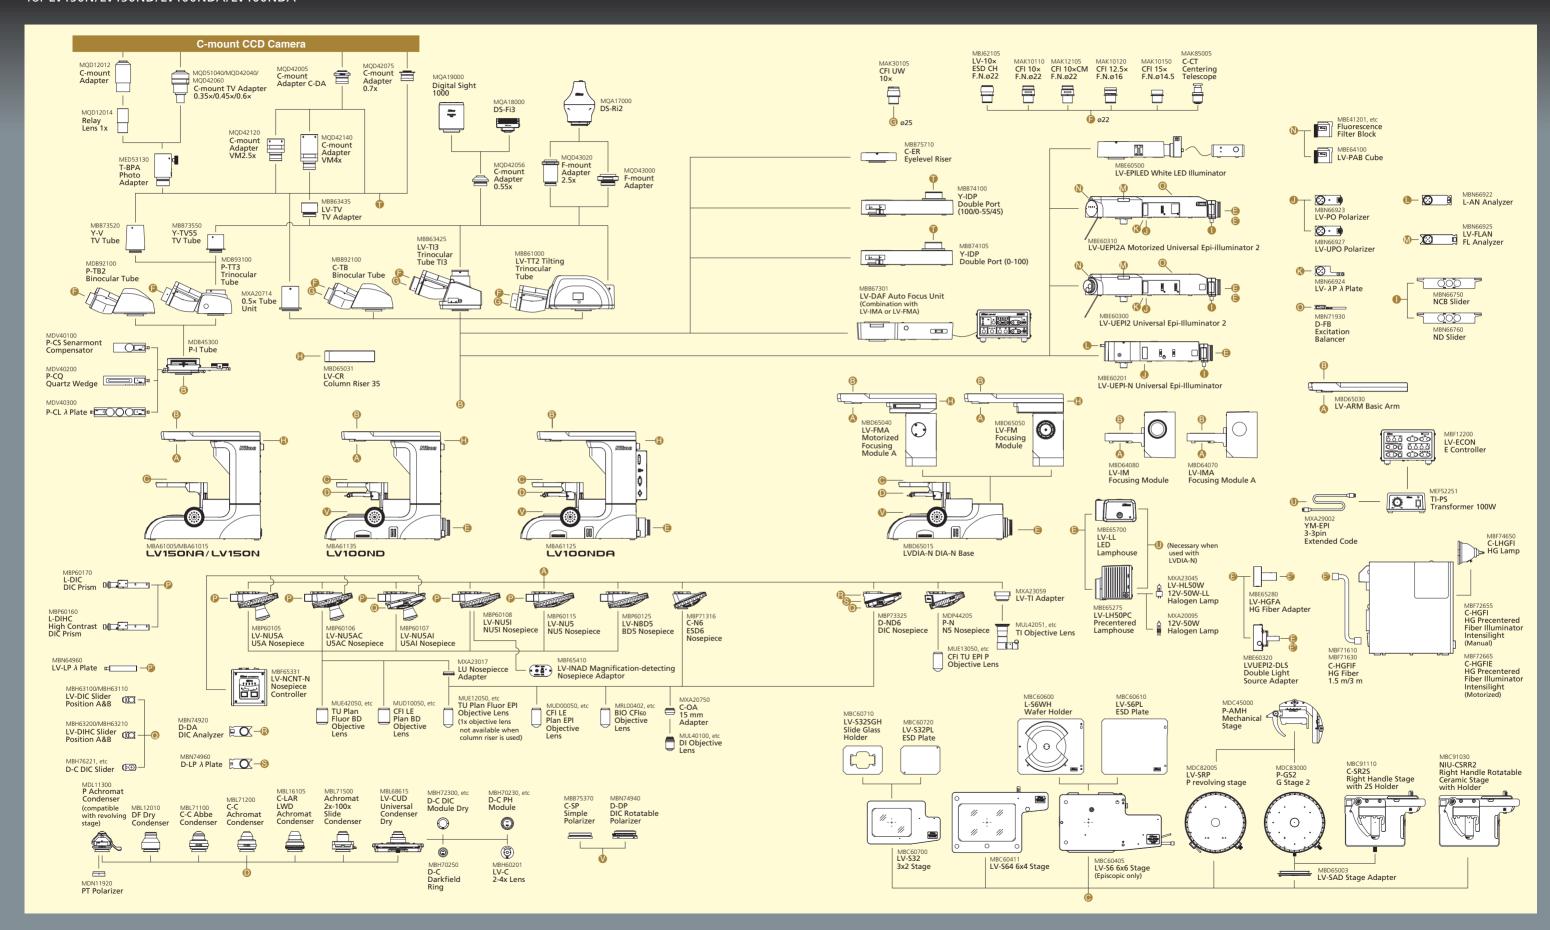

14 15

System Diagram

for LV150NL

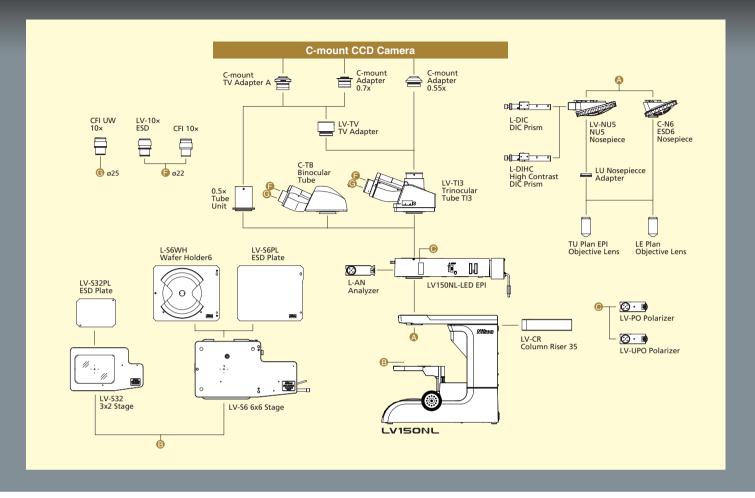

Specifications and equipment are subject to change without any notice or obligation on the part of the manufacturer. July 2020 ©2012-2020 NIKON CORPORATION

N.B. Export of the products in this brochure is controlled under the Japanese Foreign Exchange and Foreign Trade Law. Appropriate export procedures shall be required in case of export from Japan. *Products: Hardware and its technical information (including software)

Company names and product names appearing in this brochure are their registered trademarks or trademarks.



TO ENSURE CORRECT USAGE, READ THE CORRESPONDING MANUALS CAREFULLY BEFORE USING THE EQUIPMENT.



NIKON CORPORATION

Shinagawa Intercity Tower C, 2-15-3, Konan, Minato-ku, Tokyo 108-6290, Japan phone: +81-3-6433-3701 fax: +81-3-6433-3784 https://www.nikon.com/products/industrial-metrology/

http://www.nikonmetrology.com/

NIKON METROLOGY EUROPE NV NIKON METROLOGY, INC.

Geldenaaksebaan 329, 3001 Leuven, Belgium phone: +32-16-74-01-00 fax: +32-16-74-01-03 E-mail: Sales.Europe.NM@nikon.com

http://www.nikonmetrology.com/en-gb NIKON METROLOGY UK LTD.

UNITED KINGDOM phone: +44-1332-811-349 fax: +44-1332-639-881

E-mail: Sales.UK.NM@nikon.com

NIKON METROLOGY SARL

FRANCE phone: +33-1-60-86-09-76 fax: +33-1-60-86-57-35 E-mail: Sales.France.NM@nikon.com

NIKON METROLOGY GMBH

GERMANY phone: +49-6023-91733-0 fax: +49-6023-91733-229

E-mail: Sales.Germany.NM@nikon.com

NIKON INSTRUMENTS S.p.A.

ITALY phone: +39-055-300-96-01 fax: +39-055-30-09-93

12701 Grand River Avenue, Brighton, MI 48116 U.S.A. phone: +1-810-220-4360 fax: +1-810-220-4300

E-mail: Sales.NM-US@nikon.com

http://www.nikonmetrology.com/en-us

NIKON CANADA INC.

CANADA phone: +1-905-602-9676 fax: +1-905-602-9953

NIKON MEXICO- Metrology Showroom

MEXICO phone: +52 (442) 688 50673

E-mail: Sales.NM-MX@nikon.com

NIKON INSTRUMENTS (SHANGHAI) CO., LTD.

CHINA (Shanghai branch) phone: +86-21-6841-2050 fax: +86-21-6841-2060 (Beijing branch) phone: +86-10-5831-2028 fax: +86-10-5831-2026 (Guangzhou branch) phone: +86-20-3882-0551 fax: +86-20-3882-0580

NIKON INSTRUMENTS KOREA CO., LTD.

KOREA phone: +82-2-2186-8400 fax: +82-2-555-4415

NIKON SINGAPORE PTE LTD.

SINGAPORE phone: +65-6559-3651 fax: +65-6559-3668 E-mail: NSG.Industrial-sales@nikon.com

ISO 14001 Certified for NIKON CORPORATION

ISO 9001 Certified for NIKON CORPORATION **Industrial Metrology Business Unit**

NIKON MALAYSIA SDN BHD

MALAYSIA phone: +60-3-7809-3688 fax: +60-3-7809-3633

PT. NIKON INDONESIA


INDONESIA phone: +62-267-864-3949 fax: +62-267-864-3950 E-mail: PTN.Instruments@nikon.com

NIKON SALES (THAILAND) CO., LTD.

THAILAND phone: +66-2633-5100 fax: 66-2633-5191

NIKON INDIA PRIVATE LIMITED

INDIA phone: +91-124-4688500 fax: +91-124-4688527



2CE-KHOH-9